



## Introduction

Most people involved in core analysis know that NMR (Nuclear Magnetic Resonance) has been part of the available suite of well logging measurements since the mid-90s, and that it is also used for routine laboratory core analysis – in part for calibration of NMR well logs. But how many people really know how NMR works, and the full extent of what it can do for the core analyst? Most core analysts know that NMR can determine porosity and pore size distributions easily and quickly, but what about fluid mobility such as Bound Volume Irreducible (BVI), Free Fluid Index (FFI), Clay Bound Water (CBW), and effective porosity? Furthermore, what about permeability, capillary pressure, and oil/water or gas/water contents? NMR can measure all these parameters quickly and accurately, and current software makes it possible to do so without extensive knowledge of NMR.

This note is an attempt to introduce NMR and these capabilities to the non-NMR expert petrophysicist and core analyst.

## Technical background

Essentially, NMR signals are generated from liquids (oil or brine) when the sample is placed in a magnetic field and then excited with a brief pulse of radio frequency (RF) energy. Immediately after the pulse, an NMR signal appears, which then dies away with a characteristic relaxation time or decay rate known as  $T_2$ . The amplitude of the signal immediately after the pulse is an indication of the total amount of fluid present, while the  $T_2$  of the signal gives valuable information about the physical environment of the liquids.

In pores filled with a single fluid, there are two main components to the NMR signal – one coming from the fluid far from the pore walls, and the other from fluid close to the pore walls. Fluids far from the pore walls give NMR signals similar to those from bulk fluids, with relatively long relaxation times, while fluids close to the pore walls undergo a process of adsorption and desorption with the pore walls which has the effect of dramatically reducing their NMR relaxation times.




# NMR and Core Analysis





In large pores, the dominant effect is from the bulk fluids, so larger pores tend to have longer NMR relaxation times. In smaller pores, the surface-to-volume ratio is much higher, so the fluids close to the pore walls tend to dominate the NMR signal, and smaller pores show overall shorter NMR relaxation times. This process is illustrated in the figures below.




Fluids in large pores have long  $T_2$  decay times, like bulk fluids

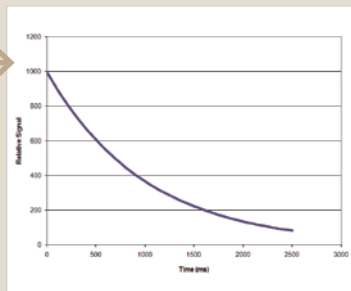


Signals from fluids in smaller pores are modified by surface interactions

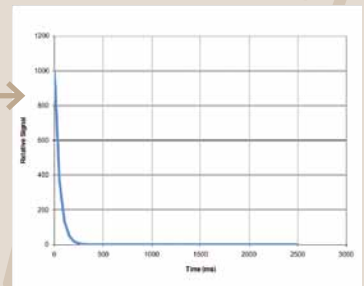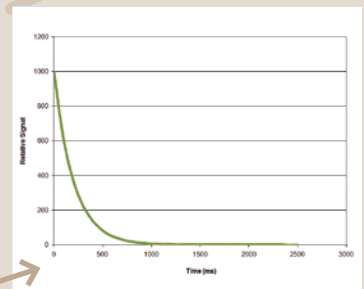



Of course, in a real measurement it is not possible to take NMR measurements from individual pores. The whole core must be measured at once, so the resulting NMR signal is a composite of all the NMR signals from the different pore sizes in the core.



+




+

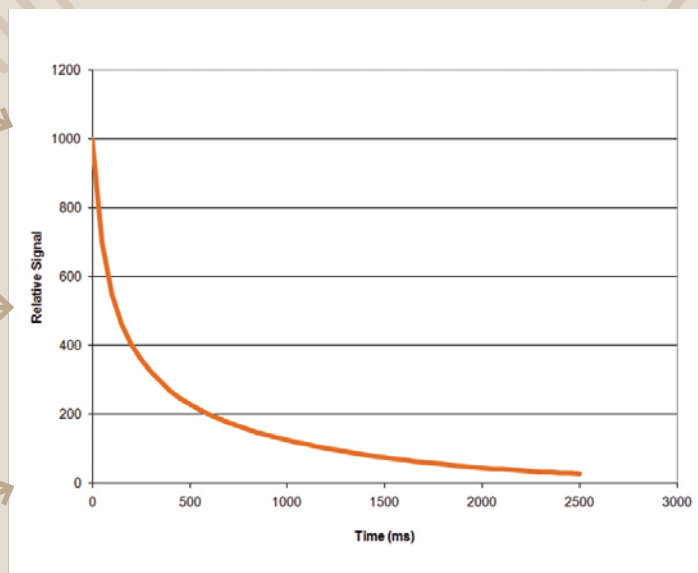




The next step is to use a mathematical procedure known as an inversion to process the composite NMR signal and separate it out into its component parts. In theory, there is one  $T_2$  component for each different pore size in the core. But in practice, the analysis is usually restricted to a maximum of about 256 individual  $T_2$  components, which is more than adequate for most practical purposes. The result of the inversion process is a  $T_2$  distribution showing the relative population of the individual  $T_2$  decay times that make up the composite NMR signal from the core. Because long  $T_2$ s come from large pores, and short  $T_2$ s from small pores, this  $T_2$  distribution is in effect a model of the pore size distribution in the core.

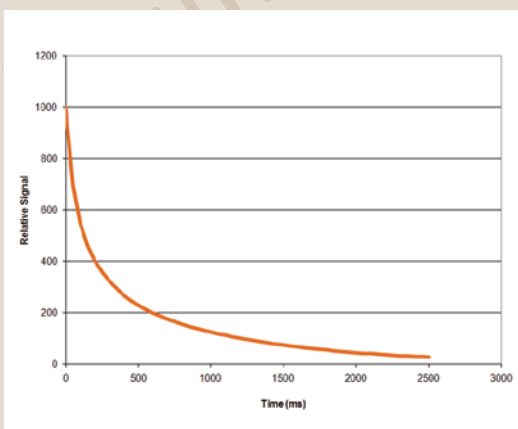


Inversion

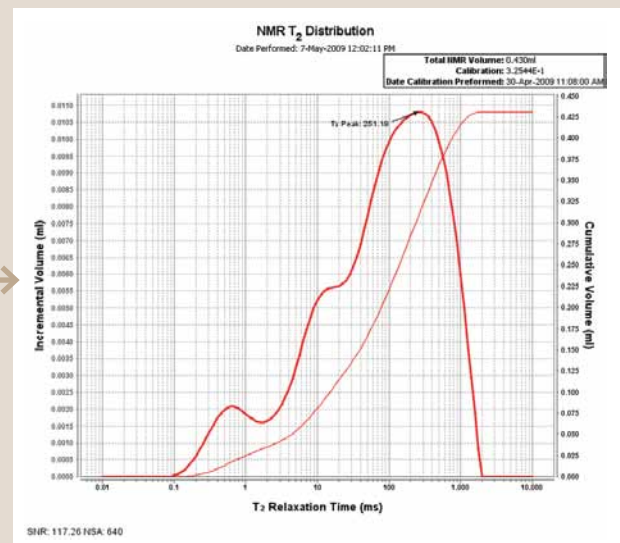

**Beyond the  $T_2$ /pore size distribution – porosity, BVI, FFI, CBW and permeability**


Once we have the basic pore size distribution from the NMR data, a number of useful petrophysical parameters can be quickly and easily inferred. The integral of all the  $T_2$ s (area under the curve) gives us the total porosity when compared to the signal from a known reference. If we centrifuge the core and then repeat the NMR measurement, the integral of the second data set is the irreducible fluid (BVI), while the difference between the two is the Free Fluid Index (FFI).

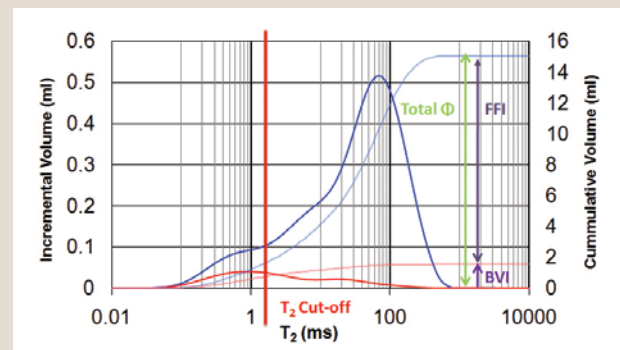

# NMR and Core Analysis



It is very important to note that the area under the saturated  $T_2$  distribution curve (which gives us a measure of total porosity) is of course influenced by the shape of the curve. If the  $T_2$  curve does not represent all the  $T_2$ s present in the sample, then signal from some pores will be missing and porosity will be under-reported. This situation can occur, for example, if the instrument being used is not capable of detecting short  $T_2$  signals from small pores, in which case porosity due to small pores will not be accounted for. Technically, this means that the instrument being used must be able to perform sustained measurements using short Time-to-Echo (TE) values. This effect is illustrated in the following figure, which shows three  $T_2$  distributions obtained on the same core sample with TE=100 $\mu$ s (green), 200 $\mu$ s (red) and 600 $\mu$ s (blue).

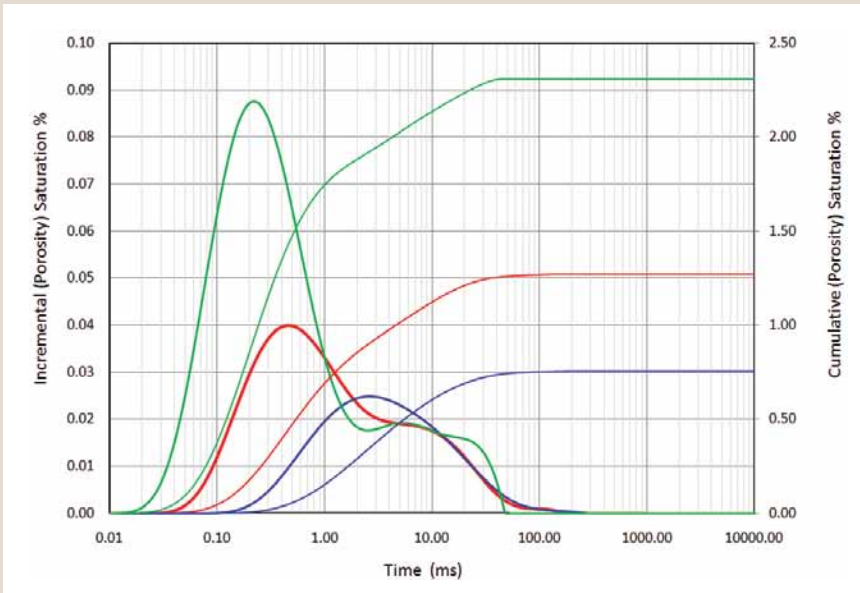

It is clear that the green (TE=100  $\mu$ s) and the red (TE=200  $\mu$ s) distributions show more detail at the shorter  $T_2$  values (smaller pores) than does the blue distribution (TE=600  $\mu$ s). The green distribution also records a much higher total integral signal, corresponding to a higher porosity value. The results are summarised in the following table:

Sample	TE ( $\mu$ s)	Acquisition Time (min)	Number of Scans	Signal to Noise Ratio	NMR Porosity (ml)
1-4R	100	2	80	220.18	4.248
	200	5.5	224	203.06	2.175
	600	21.5	864	200.16	1.151

It is standard practice nowadays to assume that all  $T_2$ s of 2.5 ms or less come from clay bound water, so these can be integrated separately to report CBW, and thence Effective Porosity.



Finally, using either the Coates or the Schlumberger model, permeability can be estimated from the relaxation data. All of these calculations are carried out and reported automatically by the LithoMetrix software incorporated in every **GeoSpec2** instrument – and the NMR measurement is non-destructive and much faster than conventional methods of obtaining the same parameters.

### There's more – Capillary Pressure, Pore Throat Distribution, Wettability and Fluid Typing


By adding an accessory called Pulsed Field Gradients (pfg) to the NMR instrument, it becomes possible to carry out measurements dependent on the diffusion, flow, or distribution of the fluids within the core sample. As with the standard measurements discussed above, integrated software controls the NMR instrument to deliver pfg-based measurements without expert knowledge of the NMR theory behind the measurements.

### Capillary Pressure

One of the more exciting recent developments in the use of NMR for core analysis is the ability to measure Capillary Pressure. Measurements that took weeks or months by special centrifuge or porous plate can now be done by NMR in hours or days – and with many times more data points.


The patented GIT-CAP technique is available in Green Imaging Technologies software offerings, which are available exclusively on Oxford Instruments' GeoSpec instrument range. GIT-CAP uses a combination of conventional centrifuge and a technique called 1-D Profiling, which is a simple version of MRI (Magnetic Resonance Imaging) that records NMR signals in one dimension only – along the axis of the core.

Here's how it works. After saturating a core, a 1-D profile measurement is acquired via the NMR instrument. The result is usually a more-or-less uniform distribution of fluid along the length of the core, as seen in the figure top right.

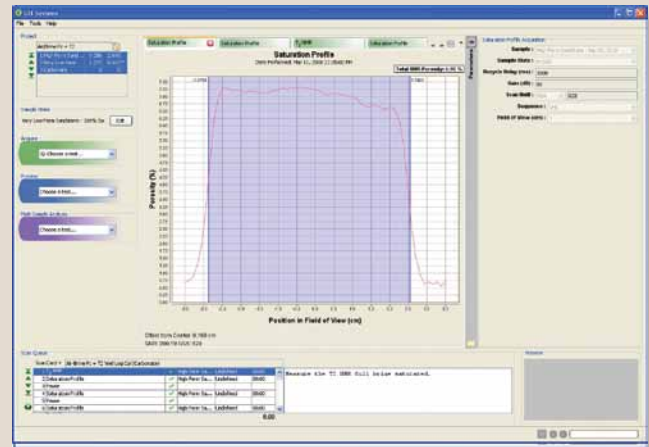

The 1-D profile records fluid saturation at between 30 and 40 points along the length of the core

The core is then spun in a standard centrifuge, which has the effect of shifting the fluid distribution towards the outer end of the core, and another 1-D profile with 30 – 40 points is obtained.

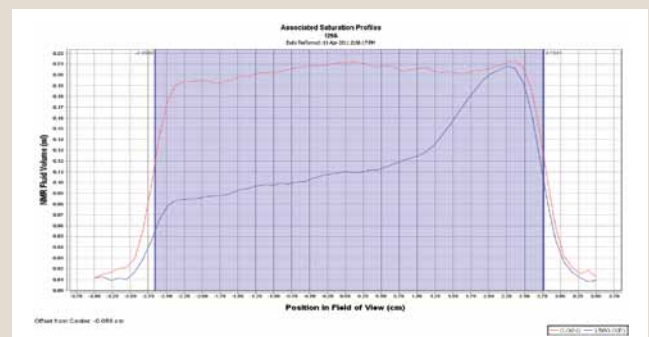


Saturation profiles before and after the first centrifugation

This process is repeated at one more centrifuge spin speed, then the data is analysed. Capillary pressure is calculated from knowledge of the centrifuge spin speeds and the changes in the saturation profile.



# NMR and Core Analysis

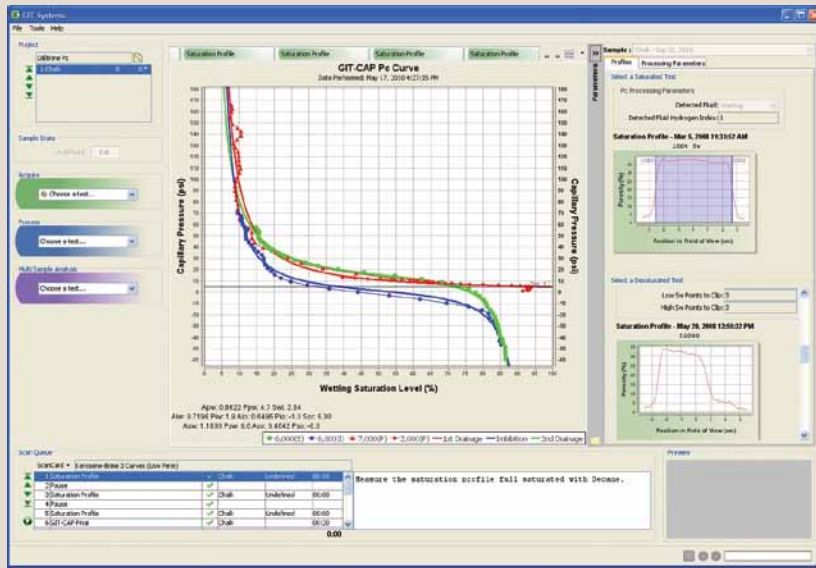


Primary drainage, imbibition, and secondary drainage capillary pressure curve

Several points are important to note in this process:

1. Only two centrifuge speeds are required, compared to eight in a traditional centrifuge Pc measurement, so four times more samples can be measured in a given time.
2. Each saturation profile yields 30 – 40 data points along the core sample instead of just one per spin speed in the traditional method. So typically 10 times more data points are collected in the NMR method.
3. The NMR method uses a standard centrifuge without stroboscope or fluid collection measurement, so the centrifuge itself is likely to be less expensive.

## Pore Throat Distribution and Wettability

Having obtained a Pc curve, pore throat distributions can now be calculated using the Washburn equations. The imbibition and secondary drainage curves generated by the NMR Pc measurement also allow USBM wettability to be predicted. Both of these calculations are integrated into the software, and follow as a natural consequence of the NMR Pc data. A further added advantage is that the NMR measurement is non-destructive and can use reservoir fluids and reservoir wettability.

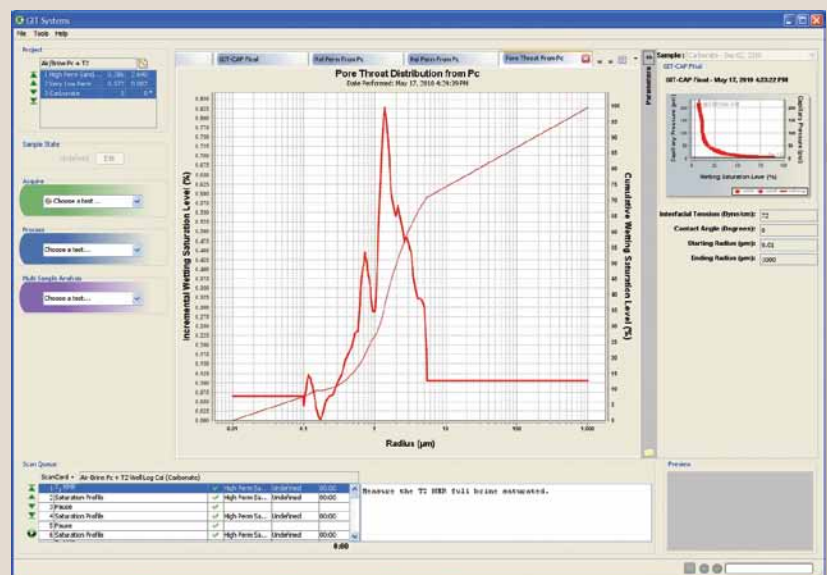


Pore throat distribution obtained from Pc data



## Fluid Typing

It was mentioned earlier that the **GeoSpec2** instruments fitted with Pulsed Field Gradients (pfg) are able to carry out measurements dependent on the diffusion, flow, or distribution of the fluids within the core sample. One application of this is for fluid typing.

It is possible that different fluids, such as heavy oils and partially bound water, may exhibit similar  $T_2$  values, which makes it difficult to identify which fluid is which using a standard  $T_2$  distribution. However, even if they have similar  $T_2$  values they are unlikely also to have similar diffusion characteristics, so a measurement that collects both  $T_2$  and diffusion data should in principle be able to separate the fluid types. **GIT Systems** software, together with a pfg accessory on a **GeoSpec2** NMR instrument, enables such measurements to be done. The result is a two-dimensional data map illustrating the relative proportions of the different fluid types in the sample.

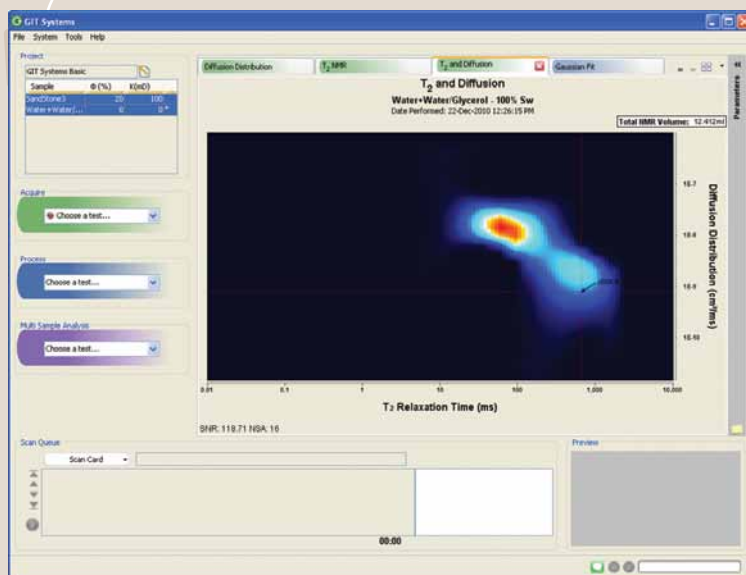

Diffusion  $T_2$  map

## Conclusions

NMR is now a well established core analysis tool, capable of making a wide range of core measurements, from pore size distributions to capillary pressure, on a single instrument. The recent partnership between Oxford Instruments and Green Imaging Technologies allows an integrated hardware and software solution to be offered to core analysts so that this wide range of applications can be covered by technicians with no specialised knowledge of NMR technology.

# GeoSpec2 – The new approach to core analysis using NMR



## Oxford Instruments Magnetic Resonance

For more than 15 years, Oxford Instruments has been the industry standard for NMR instrumentation for core analysis. With over a hundred installations, Oxford Instruments truly understands the needs of core analysts, whether they be in oil companies, oilfield service companies or academia.

Innovation has been the driving force behind Oxford Instruments' growth and success ever since the business spun out from the University of Oxford over 50 years ago. It is now a global company with over 1,300 staff worldwide and a listing on the London Stock Exchange (OXIG).

## Green Imaging Technologies

Green Imaging Technologies is committed to providing innovative solutions for lab-based analysis of rock core via Nuclear Magnetic Resonance (NMR). GIT's products and services offer fast, accurate, non-destructive analysis of rock core samples used by the oil and gas industry in exploration and reservoir characterization.

Beginning with a patented capillary pressure measurement technique in 2005, GIT has the goal of making NMR core analysis more accessible and expanding the analysis that can be done with NMR. GIT's product offerings have evolved and expanded to include a full suite of routine and advanced core analysis tools. A culture of continual innovation has driven the company to be the industry leader in NMR core analysis.



## Oxford Instruments Magnetic Resonance

For more information: [magres@oxinst.com](mailto:magres@oxinst.com)  
[www.oxford-instruments.com](http://www.oxford-instruments.com)

### UK

Tubney Woods, Abingdon, Oxfordshire, OX13 5QX, UK  
**Tel:** +44 (0) 1865 393 200 **Fax:** +44 (0) 1865 393 333

### USA

300 Baker Avenue, Suite 150, Concord, MA, 01742, USA  
**Tel:** +1 978 369 9933 **Fax:** +1 978 369 8287

### China

Room 1/E, Building 1, Xiangzhang Garden  
No. 248 Donglan Road, Shanghai 201102, China  
**Tel:** +86 21 6073 2925 **Fax:** +86 21 6360 8535

## Green Imaging Technologies

For more information: [info@greenimaging.com](mailto:info@greenimaging.com)  
[www.greenimaging.com](http://www.greenimaging.com)

### Canada

2024 Lincoln Road, Fredericton, NB, Canada, E3B 8M7  
**Toll Free:** +1 888 944 8462  
**Tel:** +1 506 458 9992 **Fax:** +1 506 458 9615

This publication is the joint copyright of Oxford Instruments and Green Imaging Technologies and provides outline information only which (unless agreed by the companies in writing) may not be used, applied or reproduced for any purpose or form part of any order or contract or be regarded as a representation relating to the products or services concerned. Oxford Instruments and Green Imaging Technologies acknowledge all trademarks and registrations. Oxford Instruments' policy is one of continued improvement. The company reserves the right to alter, without notice, the specification, design or conditions of supply of any product or service. Ref: CA-TN-04-11

